



University of  
**Salford**  
MANCHESTER

# Compression force variability in mammography in Ghana – a baseline study

Dzidzornu, E, Angmorterh, SK, Ofori-Manteaw, BB, Aboagye, S, Ofori, EK, Owusu-Agyei, S and Hogg, P

<http://dx.doi.org/10.1016/j.radi.2020.07.007>

<b>Title</b>	Compression force variability in mammography in Ghana – a baseline study
<b>Authors</b>	Dzidzornu, E, Angmorterh, SK, Ofori-Manteaw, BB, Aboagye, S, Ofori, EK, Owusu-Agyei, S and Hogg, P
<b>Type</b>	Article
<b>URL</b>	This version is available at: <a href="http://usir.salford.ac.uk/id/eprint/57759/">http://usir.salford.ac.uk/id/eprint/57759/</a>
<b>Published Date</b>	2021

USIR is a digital collection of the research output of the University of Salford. Where copyright permits, full text material held in the repository is made freely available online and can be read, downloaded and copied for non-commercial private study or research purposes. Please check the manuscript for any further copyright restrictions.

For more information, including our policy and submission procedure, please contact the Repository Team at: [usir@salford.ac.uk](mailto:usir@salford.ac.uk).

# **COMPRESSION FORCE VARIABILITY IN MAMMOGRAPHY IN GHANA – A BASELINE STUDY.**

Elizabeth Dzidzornu<sup>1</sup>, Seth Kwadjo Angmorterh<sup>1&</sup>, Bismark Bright Ofori-Manteaw<sup>1</sup>, Sonia Aboagye<sup>2</sup>, Eric Kwasi Ofori<sup>1</sup>, Seth Owusu-Agyei<sup>3</sup>, Peter Hogg<sup>4</sup>.

## **Addresses**

<sup>1</sup>Department of Medical Imaging, School of Allied Health Sciences, University of Health and Allied Sciences (UHAS), Ho, Ghana.

<sup>2</sup>Department of Speech, Language & Hearing Sciences, School of Allied Health Sciences, University of Health and Allied Sciences (UHAS), Ho, Ghana.

<sup>3</sup>Institute of Health Research (IHR), University of Health and Allied Sciences (UHAS), Ho, Ghana.

<sup>4</sup>Department of Radiography, School of Health and Society, Frederick Road Campus, University of Salford, Manchester, United Kingdom.

## **Twitter handles**

Seth Kwadjo Angmorterh - @SethKwadjo

Elizabeth Dzidzornu - @BettyManteaw

Bismark Bright Ofori-Manteaw - @brytebarca

Peter Hogg - @p\_peterhogg

## **&Corresponding author**

Dr. Seth Kwadjo Angmorterh

Department of Medical Imaging, School of Allied Health Sciences, University of Health and Allied Sciences (UHAS), Ho, Ghana.

Email: [sangmorterh@uhas.edu.gh](mailto:sangmorterh@uhas.edu.gh) Tel: +233556441769

# **1 Abstract**

## **Introduction**

Breast compression during mammographic examinations improves image quality and patient management. Several studies have been conducted to assess compression force variability among practitioners in order to establish compression guidelines. However, no such study has been conducted in Ghana. This study aims to investigate the compression force variability in mammography in Ghana.

## **Methods**

This retrospective study used data gathered from 1,071 screening and diagnostic mammography patients from January, 2018-December, 2019. Data were gathered by seven radiographers at three centers. Compression force, breast thickness and practitioners' years of work experience were recorded. Compression force variability among practitioners and the correlation between compression force and breast thickness were investigated.

## **Results**

Mean compression force values recorded for craniocaudal (CC) (17.2 daN) and mediolateral oblique (MLO) (18.2 daN), were within the recommended values used by western countries. Most of the mammograms performed – 80% – were within the National Health Service Breast Screening Programme (NHSBSP) range. However, 65% were above the Norwegian Breast Cancer Screening Programme (NBCSP) range. Compression forces varied significantly ( $p=0.0001$ ) among practitioners. Compression forces increased significantly ( $p=0.0001$ ) with the years of experience. A weak negative correlation ( $r=-0.144$ ) and a weak positive correlation ( $r=0.142$ ) were established between compression force and breast thickness for CC and MLO projections respectively.

## **Conclusion**

This initial study confirmed that although wide variations in compression force exist among practitioners in Ghana, most practitioners used compression forces broadly within the range set by the NHSBSP. As no national guidelines for compression force currently exist in Ghana, provision of these may help to reduce the range of variations recorded.

### **Implications for practice**

Confirmation of variations in compression will guide future practice to minimise image quality disparities and improve quality of care.

## 2 Introduction

Mammography is the most widely used medical imaging modality for breast cancer screening and detection.<sup>1</sup> To achieve a diagnostically acceptable mammogram, adequate compression of the breast is required.<sup>2</sup> To achieve uniform breast tissues, breast compression is applied to decrease the thickness of the breast.<sup>3,4</sup> Studies<sup>5,6</sup> have shown that breast compression and its impact on reducing breast thickness has a positive effect in reducing radiation exposure to the patient. Furthermore, compression of the breast improves image quality by reducing motion artifacts and image blurring due to the ability of the compression paddles to firmly hold the breast in a specific position.<sup>7,8</sup> The clinical benefits of breast compression are that it enhances breast cancer detection, thereby improving patient management.<sup>9</sup> However, the application of breast compression force varies across and within practitioners,<sup>9,10</sup> and in some cases may lead to pain,<sup>11,12</sup> and deter patients from attending future breast screening examinations.<sup>13</sup>

Several countries have produced breast compression guidelines for radiographers to apply during mammography examinations. The United Kingdom (UK) National Health Service Breast Screening Programme (NHSBSP) guidelines recommend that compression force should not exceed 20 decanewton (daN) and that compression should be applied slowly and gently to ensure that the breast is firmly held in position.<sup>14</sup> Similarly, the Norwegian Breast Cancer Screening Program (NBCSP) recommends a breast compression force range between 10.8-17.7 daN,<sup>15</sup> while the quality assurance guidelines for mammography in the United States (US) recommend a breast compression force between 11-20 daN.<sup>16</sup> The European guidelines recommend between 13-20 daN with the breast to be firmly compressed, yet tolerable for the patient.<sup>17</sup> Despite the existence of these recommendations, variations in the application of compression force by imaging professionals continues to be reported across studies<sup>9,10,18,19</sup>, between centers<sup>6,15,19</sup> and across countries<sup>20</sup>. A common feature across studies is that the compression force which is applied tends to be practitioner dependent rather than patient dependent.

Currently, no specific compression force guidelines exist in Ghana. Neither have any previous studies been conducted to assess the breast compression force applied during mammography procedures by Ghanaian practitioners. The purpose of this study is to investigate the possible variations in compression force used among practitioners in Ghana to serve as a baseline data for future studies and contribute to the formation of national compression force guidelines.

### 3 Methods

Ethical approval was received from the Research and Ethics Committee of the University of Health and Allied Sciences, Ho, Ghana. Permission was also sought from the breast centers involved in the study. A purposive sampling technique was used to select three mammography centers for this study. In total, there are five digital mammography centers in Ghana. The absence of a national breast screening programme, coupled with limited data on national breast cancer screenings in Ghana<sup>21-23</sup>, influenced the selection of these breast centers since they were the major breast screening centers with functional mammography machines at the time of data collection. Also, these centers were chosen because their quality control (QC) programmes were within the manufacturers' tolerances. Each breast center had one stationary Fujifilm FDR-2500DRLA digital mammography machine.

The study utilized retrospective data from a total of 1,071 patients, aged 35 years and above, who visited any of the three mammography centers for either screening or diagnostic mammography within the periods of January, 2018 to December, 2019. Parameters such as compression force in decanewton (daN) and compressed breast thickness in millimeters (mm), age of patients and practitioners' identity and years of work experience were obtained from the mammography information system. Data was entered manually into the Statistical Package for the Social Sciences (SPSS) version 23. Before the performance of each examination, the details of the patient were entered into the database alongside a unique identifier for the practitioner doing the examination. This facilitated easy identification of examinations conducted by each practitioner. Seven qualified practitioners (two from center one and two, and three from center three) performed the examinations. The practitioners were coded 1-7 and the mammography centers 1-3 for anonymity. The practitioners were all qualified radiographers, had additional training in mammography, and mammography was part of their normal job.

The study excluded 17 patients (68 mammograms) with incomplete data, three patients (12 mammograms) with breast implants, 18 patients (118 mammograms) with more than the four standard mammographic projections, and 54 patients (120 mammograms) with less than the four standard mammographic projections. In total, four-view mammography images (left craniocaudal, left mediolateral oblique, right craniocaudal, and right mediolateral oblique) from 979 patients, resulting in 3,916 mammograms were included in the study.

Compression forces between the right and left breast showed no statistical significance ( $p = 0.913$ ). Therefore, the values of the right breast were used in the analysis to enable simplification of the results. The data was subjectively assessed for normality by visual observation using histograms, stem and leaf. It was objectively assessed using the Kolmogorov Smirnov (KS) test. The subjective analysis showed that the data was not normally distributed. Similarly, the KS test results showed a statistically significant p-value ( $p = 0.0001$ ) indicating that the data was not normally distributed. Consequently, non-parametric statistics were conducted for inferential statistics. The mean compression force recorded was tabulated against recommended mammographic compression guidelines in other countries. The non-parametric Kruskal Wallis test was conducted to assess the breast compression forces applied between practitioners. Pairwise comparison using the Bonferroni confidence interval (CI) adjustment was also conducted to control for type 1 error. In instances where there was a statistically significant difference between the breast compression force among the practitioners, post-hoc Wilcoxon rank tests were conducted to determine exactly where the differences occurred. Spearman's rho correlation coefficient ( $r$ ) was used to determine the correlation between the compression force and compressed breast thickness. The coefficient of determination ( $R^2$ ) was calculated by multiplying  $r$  by itself and expressing it as a percentage. Cohen's<sup>24</sup> interpretation of  $r$  was used to interpret the strength of the correlation;  $r=0.1-0.29$  (small),  $r=0.30-0.49$  (medium), and  $r=0.50-1.0$  (large).

## 4 Results

In all, four standard mammographic images each (left craniocaudal, left mediolateral oblique, right craniocaudal, and right mediolateral oblique) from 979 patients, resulting in 3,916 mammograms were used for data analysis. The patients were aged between 35 and 87 years [mean = 54 years; standard deviation (SD) = 10.0]. The years of work experience of the practitioners ranged between two to 10 years [mean = 6; SD = 2.8]. The number of cases per practitioner per center are indicated in table 1.

Table 1: The number of cases per practitioner per center

<b>Centers</b>	<b>Practitioner ID</b>	<b>Frequency [Percent (%)] per practitioner</b>	<b>Frequency [Percent (%)] per center</b>
<b>Center one</b>	Practitioner 1	122 (12.5)	204 (20.9)
	Practitioner 2	82 (8.4)	
<b>Center two</b>	Practitioner 3	172 (17.6)	310 (31.7)
	Practitioner 4	138 (14.1)	
<b>Center three</b>	Practitioner 5	103 (10.5)	465 (47.5)
	Practitioner 6	165 (16.9)	
	Practitioner 7	197 (20.1)	
	<b>Total</b>	<b>979 (100)</b>	<b>979 (100)</b>

The mean breast compression force values for craniocaudal (CC) and mediolateral oblique (MLO) and standard deviation were  $17.24 \pm 3.6$  daN and  $18.19 \pm 3.1$  daN respectively. The breast compression force values obtained in this study are compared with the recommended breast compression force ranges in other countries (table 2). The mean compressed breast thickness recorded was  $36.06 \pm 11.7$  mm for CC and  $44.64 \pm 14.4$  mm for MLO.



Table 2: Comparison of mean breast compression force to international recommended values

<b>TOTAL</b>		Mean±SD (in daN)			
Cranio-caudal (CC) projection		17.24 ± 3.6 daN			
Mediolateral oblique (MLO) projection		18.19 ± 3.1 daN			
		<b>NHSBSP – UK (&lt; 20 daN)</b>	<b>NBCSP – Norway (10.8–17.7 daN)</b>	<b>US (11– 20 daN)</b>	<b>Europe (13–20 daN)</b>
<b>Total</b>	Mammograms below range	-	4.7 % (186/3916)	5% (195/3916)	8.1 % (316/3916)
	Mammograms within range	80 % (3131/3916)	37.5 % (1469/3916)	75 % (2936/3916)	71.9 % (2815/3916)
	Mammograms above range	20 % (785/3916)	57.7 % (2261/3916)	20 % (785/3916)	20 % (785/3916)
<b>Center one</b>	Mammograms below range	-	0.9 % (7/816)	0.9 % (7/816)	0.9 % (7/816)
	Mammograms within range	28.2 % (230/816)	5.1 % (42/816)	27.3 % (223/816)	27.3 % (223/816)
	Mammograms above range	71.8 % (586/816)	94 % (767/816)	71.8 % (586/816)	71.8 % (586/816)
<b>Center two</b>	Mammograms below range	-	3 % (37/1240)	3.1 % (39/1240)	6.1 % (76/1240)
	Mammograms within range	89.6 % (1111/1240)	46.4 % (575/1240)	86.5 % (1072/1240)	83.5 % (1035/1240)
	Mammograms above range	10.4 % (129/1240)	50.6 % (628/1240)	10.4 % (129/1240)	10.4 % (129/1240)
<b>Center three</b>	Mammograms below range	-	7.6 % (142/1860)	8.0 % (149/1860)	12.5 % (233/1860)
	Mammograms within range	96.2 % (1790/1860)	45.8 % (852/1860)	88.2 % (1641/1860)	83.7 % (1557/1860)
	Mammograms above range	3.8 % (70/1860)	46.6 % (866/1860)	3.8 % (70/1860)	3.8 % (70/1860)

The Kruskal-Wallis test results revealed a statistically significant difference ( $p = 0.0001$ ) in the breast compression forces applied in the CC projection among the seven practitioners. Similarly, the Kruskal-Wallis test results revealed a statistically significant difference ( $p = 0.0001$ ) in the breast compression forces applied in the MLO projection among the seven practitioners. The median values of each practitioner per the CC and MLO projections are shown in figures 1 and 2 respectively. Figure one is a box plot indicating variability in the compression force applied across the practitioners for the CC projection; practitioner two recorded the highest median compression force (21.9 daN) and practitioner six recorded the least median compression force (16.5 daN).

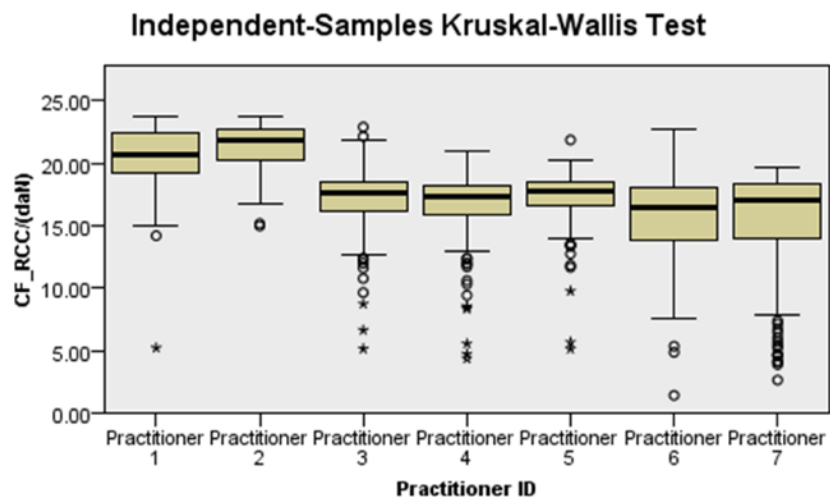


Figure 1: The median values recorded for the Kruskal Wallis test for each practitioner for the CC projection

Figure two is a box plot indicating variability in the compression force applied across the practitioners for the MLO projection; practitioner two recorded the highest median compression force (22.6 daN) and practitioners three, four, five, six and seven recorded similar median compression forces (17.9 daN).

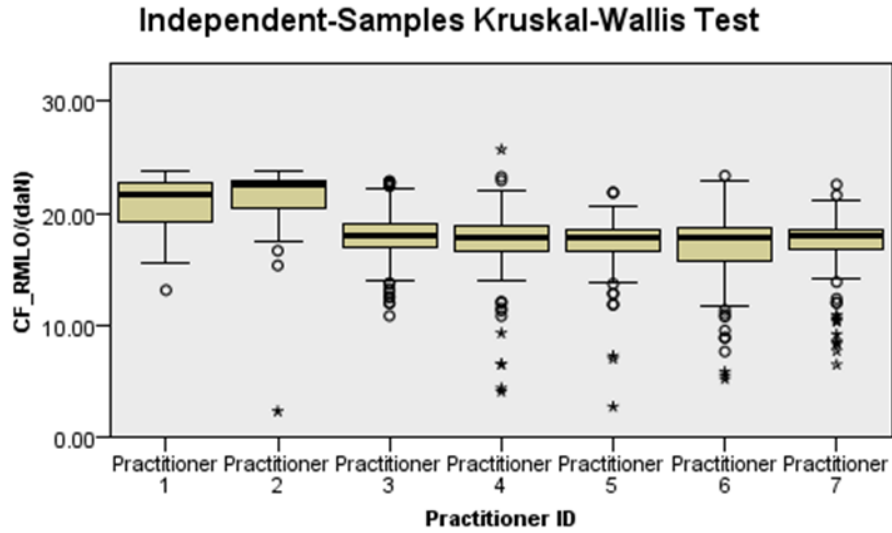


Figure 2: The median values recorded for the Kruskal Wallis test for each practitioner for the MLO projection

The results of the post-hoc pairwise comparison using the Bonferroni confidence interval (CI) adjustment, indicated that there were statistically significant differences ( $p=0.001$ ) in the breast compression force applied among the seven practitioners for both the CC and MLO projections (table 3).

Table 3: Results of post-hoc pairwise comparison indicating inconsistencies in the breast compression force applied among seven practitioners for both the CC and MLO projections

Practitioner vs. Practitioner		Significance level		Significance level
<b>P1-P3</b>	<b>CC</b>	0.001	<b>MLO</b>	0.001
<b>P1-P4</b>		0.001		0.001
<b>P1-P5</b>		0.001		0.001
<b>P1-P6</b>		0.001		0.001
<b>P1-P7</b>		0.001		0.001
<b>P2-P3</b>		0.001		0.001
<b>P2-P4</b>		0.001		0.001
<b>P2-P5</b>		0.001		0.001
<b>P2-P6</b>		0.001		0.001

<b>P2-P7</b>		0.001		0.001
<b>P3-P6</b>		0.011		0.001
<b>P3-P7</b>		0.020		0.047
<b>P4-P6</b>		0.001		0.010
<b>P5-P6</b>		0.020		0.003

\*P = practitioner

Spearman's rho correlation coefficient indicated a weak negative correlation between the breast compression force and compressed breast thickness for the CC projections ( $r = -0.144$ ), and a weak positive correlation between breast compression force and compressed breast thickness for the MLO projection ( $r = 0.142$ ). The coefficient of determination showed 2.1 % and 2.0 % shared variance between breast compression force and compressed breast thickness for the CC and MLO respectively. Similarly, there was a weak positive correlation between the breast compression force and practitioners' years of work experience ( $r = 0.247$  for CC and  $r = 0.171$  for MLO). There was no correlation between the compression force and age of patients ( $r = 0.077$  for CC and  $r = 0.009$  for MLO).

## 5 Discussion

This study compared breast compression force and compressed breast thickness applied during four-view mammography by practitioners across three test centers in Ghana. All the study participants were females and their mean age mean ( $54 \pm 10.0$ ) was within the common age for breast cancer screening.<sup>25</sup> This was similar to the age range reported by a study profiling Ghanaian mammography patients ( $51 \pm 8.9$ ).<sup>21</sup> In the current study, the mean compressed breast thickness recorded for the craniocaudal (CC) was  $36.06 \pm 11.7$  mm, and the mediolateral oblique (MLO) was  $44.64 \pm 14.4$  mm; these values were lower than those recorded by Moshina et al.<sup>26</sup> in Norway [ $56.9 \pm 12.0$  mm (CC);  $60.0 \pm 13.7$  mm (MLO)]. The differences in the recorded compressed breast thickness could be due to differences in breast characteristics/composition such as density and size<sup>27</sup> among black African women compared to predominantly Caucasian women. The mean breast compression force applied for the CC and MLO projections in this study were within the recommended values detailed by guidelines published in the UK and USA<sup>14-17</sup>. The MLO value was, however, above the NBCSP range set by Norway, as shown in table 2. The highest percentage (80%) of mammograms within the recommended guidelines of other countries were recorded for the NHSBSP (UK). In contrast, the NBCSP recorded the highest percentage (62.5%) of mammograms outside the recommended range, as evident in table 2. This indicates that the breast compression forces applied by practitioners in Ghana were more aligned to UK rather than Norwegian protocols. Ghana currently lacks national mammographic compression force guidelines. However, the values from this baseline study, alongside international guidelines, could serve as reference data to guide the formation of national recommended breast compression guidelines to guide the practice of mammography in Ghana.

The findings of this study confirmed that variations in compression force existed among mammography practitioners in Ghana. This finding is consistent with the results of previous studies.<sup>9,15,18,19,28</sup> Mercer et al.<sup>9</sup> attributed variations in the compression force to three factors: practitioner, equipment and the patient. Variations stemming from patients could be due to differences in their tolerance of pain<sup>11,12</sup>, breast density, size, stiffness and compressibility.<sup>27,29</sup> The study by Mercer et al.<sup>9</sup> categorized the breast compression force among practitioners as high, intermediate and low in relation to breast volume and density. To minimise the variations in breast compression force and reduce unnecessary pain, the use of pressure controlled paddles, taking into account compression force and breast size, to compress breasts to achieve the required pressure

for varying breast sizes has been recommended.<sup>5,8</sup> Factors relating to the practitioner include their age, years of work experience and adherence to protocols. This study recorded a statistically significant difference ( $p = 0.0001$ ) in the practitioners' years of work experience and the amount of breast compression force applied. Practitioners may rely more on their experience when applying breast compression due to the absence of Ghanaian protocols. This may contribute to the wide range of variations recorded. Consistent with the results of this current study, a previous study by Waade et al.<sup>15</sup> recorded a statistically significant difference ( $p < 0.05$ ) between the practitioners' years of work experience, age and compression force. It is in line with this that Branderhorst et al.<sup>6</sup> recommended the use of pressure standardization in the production of mammogram images. This can help to both minimise significant variations among practitioners, and enable the production of reproducible images. A further finding of this study was the variation between data across study centers. Center one had the least compliance with western protocols whilst center three had the greatest. This may be related to the fact that center one had older practitioners with several years of work experience compared to center three.

Studies<sup>28,30</sup> have reported that increased compression force decreases the compressed breast thickness. This is supported by the negative correlation ( $r = -0.144$ ) recorded in this study for the CC projection. However, the MLO projection recorded a weak positive correlation ( $r = 0.142$ ) supporting the findings of Waade et al.<sup>15</sup>. It is likely that the patient positioning during the acquisition of the MLO projection could have impacted on this positive correlation. Patient positioning during MLO projection includes the juxtathorax which are mostly thicker and stiffer than the breast tissues and could be visualized on a typical MLO projection. This position is comparable to findings by Dustler et al.<sup>31</sup> and Förnvik et al.<sup>2</sup> Although there is evidence to show that increased breast compression reduces breast thickness, over compression (the use of excessively high pressure) of the breast has little clinical benefit, in that, it has minimal effect on breast thickness reduction.<sup>32</sup> Over compression could cause pain/discomfort and could induce the development of pressure ulcers in the breast. Further analysis recorded a slight increase in the compression force in tandem with an increase in the practitioners' years of work experience. It can be inferred from the results that, as the practitioners' years of work experience increase, higher compression forces are applied. This, in turn, decreases the compressed breast thickness, motion blurring and radiation exposure to the patient and the radiographer. It also improves uniform distribution of the breast tissues to achieve optimum image quality. Förnvik et al.<sup>2</sup> suggested that

optimum breast compression force is essential for producing diagnostically acceptable images, detecting possible lesions and facilitating accurate diagnosis, thereby improving patient management. However, high levels of breast compression force could be painful to patients. The clinical implication of this is that patients could be deterred from attending future breast screening examinations. Only three mammography centers had functional digital mammography machines that met manufacturer QC recommendations at the time of the study so the results of this study should be generalized with caution.

## **6 Conclusion**

This baseline study investigated the breast compression force applied in mammography examinations in Ghana. Statistically significant differences were measured in the levels of breast compression force applied. This was due to variations in compression force used among practitioners. The years of work experience of the practitioners were significantly related to the compression force applied. The age of the patient had no effect on the amount of breast compression force applied. 80% of the mammograms reviewed in this study were within the National Health Service Breast Screening Programme (NHSBSP) of the UK while 60% were not consistent with the more stringent Norwegian Breast Cancer Screening Program (NBCSP) guidelines. There was a weak correlation recorded between breast compression force and compressed breast thickness.

## **7 Limitation and recommendation for future study**

As a baseline study, this study had small study size. A larger sample from all mammography centers in Ghana would be needed to establish whether breast compression force variability exists in Ghana, and the findings from that study will be used to inform the development of a national breast compression guidelines.

## 8 References

1. Sree SV, Ng EY-K, Acharya RU, Faust O. Breast imaging: A survey. *World J Clin Oncol.* 2011;2(4):171.
2. Förnvik D, Andersson I, Svahn T, Timberg P, Zackrisson S, Tingberg A. The effect of reduced breast compression in breast tomosynthesis: Human observer study using clinical cases. *Radiat Prot Dosimetry.* 2010;139(1–3):118–23.
3. Smith A. Improving Patient Comfort in Mammography. *Hologic.* 2017;2(1):1–8.
4. Kuppusamy T. *Basic Radiological Physics.* 2017. 1–473 p.
5. Feder K, Grunert J. Is Individualizing Breast Compression during Mammography useful ? – Investigations of pain indications during mammography relating to compression force and surface area of the compressed breast Ist eine Individualisierung der mammografischen Brustkompress. 2017;39–48.
6. Branderhorst W, Groot JE De, Highnam R, Chan A, Böhm-vélez M, Broeders MJM, et al. Mammographic compression – A need for mechanical standardization. *Eur J Radiol.* 2015;1(1):1–7.
7. Jeukens CRLPN, Dijk T Van, Berben C, Wildberger JE, Lobbes MBI. Evaluation of pressure-controlled mammography compression paddles with respect to force-controlled compression paddles in clinical practice. *Eur Radiol.* 2019;11(4):1–8.
8. De Groot JE, Broeders MJM, Branderhorst W, Den Heeten GJ, Grimbergen CA. A novel approach to mammographic breast compression: Improved standardization and reduced discomfort by controlling pressure instead of force. *Med Phys.* 2013;40(8):1–9.



9. Mercer CE, Hogg P, Lawson R, Diffey J, Denton ERE. Practitioner compression force variability in mammography: A preliminary study. *Br J Radiol.* 2013; 86(1022):1–9.
10. Murphy F, Nightingale J, Hogg P, Robinson L, Seddon D, Mackay S. Compression force behaviours: An exploration of the beliefs and values influencing the application of breast compression during screening mammography. *Radiography* 2015;21(1):30–5.
11. Askhar LK, Zaki YH. Female patients' perception of pain caused by mammography in the Western Region of Saudi Arabia. *Saudi Med Journal.* 2017;38(7):768–71.
12. Whelehan P, Evans A, Wells M, Macgillivray S. The effect of mammography pain on repeat participation in breast cancer screening : A systematic review. *The Breast.* 2013;22(4):389–94.
13. De Groot JE, Broeders MJM, Grimbergen CA, Den Heeten GJ. Pain-preventing strategies in mammography: An observational study of simultaneously recorded pain and breast mechanics throughout the entire breast compression cycle. *BioMed Cent Women's Heal.* 2015;15(1):1–9.
14. Borrelli C, Dale M, Jenkins J, Kelly J, Zoe V, Whelehan P. NHS Breast Screening Programme . Guidance for breast screening mammographers. 3rd ed. London: Public Health England; 2019. 1–37 p.
15. Waade GG, Moshina N, Sebuødegard S, Hogg P, Hofvind S. Compression forces used in the Norwegian breast cancer screening program. *Br J Radiol.* 2017;90(1071):1–21.
16. US Food and Drugs Administration. The Mammography Quality Standards Act and

- Program. *Radiol Clin North Am.* 2020;38(4):759–72.
17. Perry N, Broeders M, Wolf C de, Törnberg S, Holland R, Karsa L von. European guidelines for quality assurance in breast cancer screening and diagnosis. 4th ed. Perry N, Broeders M, Wolf C de, Törnberg S, Holland R, Karsa L von, editors. Belgium: European Union; 2013. 1–160 p.
  18. Mercer CE, Hogg P, Szczepura K, Denton ERE. Practitioner compression force variation in mammography: A 6-year study. *Br J Radiogr.* 2013;19(3):200–6.
  19. Mercer CE, Szczepura K, Kelly J, Millington SR, Denton ERE, Borgen R, et al. A 6-year study of mammographic compression force: Practitioner variability within and between screening sites. *Radiography* 2015;21(1):68–73.
  20. Ng KH, Hill ML, Johnston L, Highnam R, Tomal A. Large variation in mammography compression internationally. *Eropean Soc Radiol.* 2017;55(33):1–14.
  21. Boadu M, Sosu EK, Hasford F, Nani EK, Sackey TA, Commission E, et al. Mammography examination in ghana: preliminary survey of patients ’ profiles. *J Appl Sci Technol.* 2012;17(1):87–92.
  22. Thomas AS, Kidwell KM, Opong JK, Adjei EK, Osei-Bonsu E, Boahene A, et al. Breast Cancer in Ghana: Demonstrating the Need for Population-Based Cancer Registries in Low- and Middle-Income Countries. *J Glob Oncol.* 2017;3(6):765–72.
  23. Naku GJF, Anyanful A, Eliason S, Mohammed Adamu S, Debrah S. Pattern of Breast Cancer Distribution in Ghana: A Survey to Enhance Early Detection, Diagnosis, and Treatment. *Int J Breast Cancer* 2016;1(1):1–9.

24. Cohen JW. Statistical power analysis for the behavioral sciences. *Commun Stat Simul Comput.* 1988;39(4):860–4.
25. Burgees L. What is the link between age and breast cancer? *Med News Today.* 2019 3;1(5):1–5.
26. Moshina N, Roman M, Waade GG, Sebuødegård S, Ursin G, Hofvind S. Breast compression parameters and mammographic density in the Norwegian Breast Cancer Screening Programme. *Eur Radiol.* 2017;28(4):1662–72.
27. Hendrick RE, Pisano ED, Averbukh A, Moran C, Eric A, Yaffe MJ, et al. Comparison of Acquisition Parameters and Breast Dose in Digital Mammography and Screen-Film Mammography in the American College of Radiology Imaging Network Digital Mammographic Imaging Screening Trial. *Am J Roentgenol.* 2011;194(2):362–9.
28. Lau S, Aziz YFA, Ng KH. Mammographic compression in Asian women. *PLoS One.* 2017;12(4):1–16.
29. Khan-Perez J, Harkness E, Mercer C, Bydder M, Sergeant J, Morris J, et al. Volumetric breast density and radiographic parameters. 1st ed. Fujita H, Hara T, Muramatsu C, editors. Switzerland: Springer; 2014. 265–272 p.
30. Perry N, Broeders M, de Wolf C, Törnberg S, Holland R, von Karsa L. European guidelines for quality assurance in breast cancer screening and diagnosis. 4th ed. Perry N, Broeders M, de Wolf C, Törnberg S, Holland R, von Karsa L, editors. Belgium: International Agency for Research on Cancer; 2008. 614–622 p.
31. Dustler M, Andersson I, Förnvik D, Tingberg A. The Effect of Breast Positioning on Breast

Compression in mammography : a Pressure Distribution Perspective. SPIE Med Imaging. 2012;8313(54):1–7.

32. Hogg P, Taylor M, Szczepura K, Mercer C. Pressure and breast thickness in mammography — an exploratory calibration study. Br Journal of Radiol. 2013;86(1021).